

Weavy®

FSM & Zapper Technology

Quick Guide

Perfect WAVES

Quick Guide

You can find the latest version of this quick guide on this web page:



Discover Your Weavy®

Your Weavy® is designed to deliver FSM and Zapper protocols, making it one of the most advanced personal devices for frequency-based therapy.

FSM Technology

- Up to 4 simultaneous frequencies
- Frequencies from 0 to 1,000 Hz
- Ultra-precise frequencies

Zapper Technology

- Zapper generator from 1 to 800 KHz
- Designed for biocompatibility
- Precision-regulated microcurrent

Weavy Life Account

Your Weavy® is a tool designed to weave a connection between you and your practitioners.

Your Weavy Life subscription enables online synchronization for your Weavy®, providing :

- A record of every protocol you use.
- Access to new protocols (FSM and Zapper) provided as part of the Optimal Health programs.
- The possibility for your practitioners to monitor your progress by receiving accurate data on the progression of your symptoms.

A Weavy Life account is not required to use your Weavy®.


For more information, please visit: https://weavy.life

Battery Charging

Please make sure your Weavy® is fully charged before using it for the first time.

Connect the provided USB-C cable to the device's USB-C port and to a USB-C smartphone charger.

Using an USB Power Delivery charger will allow a fast charge of your device.

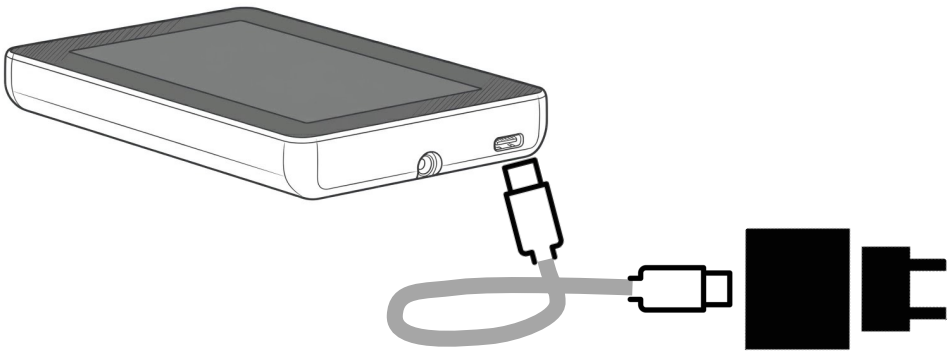


Cable Installation


Your Weavy® comes with two types of cables:

- A cable with 3.5 mm push-pin connectors
- A cable with 2 mm pin connectors

Connect the appropriate cable depending on the type of electrodes you are using.

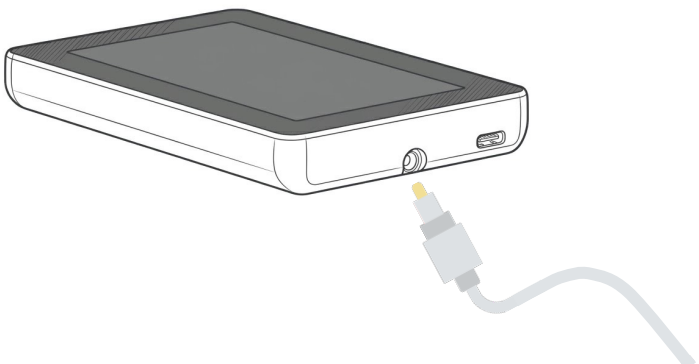

First Startup



Because your Weavy® needs to download the included protocols from Weavy Life, a Wi-Fi connection is required at first startup.

If a Wi-Fi connection is not available, you can activate the Wi-Fi hotspot feature on your smartphone.

If you have a Weavy Life account, you will be able to enter the email address and password used to create your account.

Your personalized protocols, created by your practitioners, may not be available at first startup.

Startup and Synchronization

At start-up, and every 3 days thereafter, your Weavy® will search for a Wi-Fi connection to perform synchronization. This feature can be turned off in the settings.



Synchronization is required to receive new protocols from your practitioners and to send your follow-up data (indicators and protocol usage).

A progress bar appears while your Weavy® is synchronizing.

Wi-Fi connection in progress

Downloading data from Weavy Life (new protocols)

Uploading data to Weavy Life


To skip synchronization, tap the X.

User Selection Screen

Your Weavy® supports up to 5 user accounts, in addition to the Guest profile.
Each user must use their own personal account to provide accurate follow-up data to their practitioners.

To add a new user, enter the email address and password used during the Weavy Life subscription.

The Guest profile is intended for users without an active subscription. It allows you to share your Weavy® with family and friends without affecting your follow-up data.



This icon indicates that a synchronization is required

This icon indicates that your protocols aren't ready yet (please contact your practitioner)

This icon indicates that the Weavy Life subscription is inactive

Child Users

On the https://weavy.life website, you can subscribe to child licenses.

Once a child license subscription is completed, a child account is automatically linked to your account. At the next synchronization of your Weavy®, a new account for your child will appear on the user screen.


This process is fully automatic, and you do not need to manually add a user account for your child.

To start a synchronization, swipe down to display the device settings, then tap the "Sync" button 

You can have up to 4 children accounts linked to your account.

For more information about child licenses, please visit: https://weavy.life

User Settings




To change your user settings, press and hold the User button.

You can modify the following:

- First name
- Avatar
- Email address associated with your Weavy Life subscription
- Password

From this menu, you can also delete a user account.

Device Settings



Swipe down to display the device settings.

Use these buttons to access the following settings:


Sound notifications when a protocol ends or when a lead is disconnected • Master volume and vibration.

Display user selection screen or electrode instruction screen.

Language • Automatic synchronization every 3 days • Zapper output mode.

View equipment information • Factory reset button to erase all data on your device.

Device Settings




Slide the top slider to adjust the device brightness.

When starting a protocol, a screen showing where to place the electrodes is displayed. To stop displaying this screen, disable this option in the settings.

If you are the only user of the device and do not want the User Selection screen to appear each time you start the Weavy®, disable this option in the settings.

Swipe up on the screen to exit the device settings.

Synchronization



At any time, to start a synchronization, go to the device settings, then tap the Sync button

During synchronization, your Weavy® will automatically update its firmware if a new version is available.

The Wi-Fi module is turned off once the synchronization is complete.

When the "Sync every 3 days" option is enabled, your Weavy® will automatically activate its Wi-Fi connection to check whether new protocols are available from the Weavy® Optimal Health ressources or from your practitioners.


Protocol Library

In the Protocol Library, you will find your different protocol packs:

- The Weavy® included protocols
- Your practitioners' protocols
- Protocol packs from our partners
- Optimal Health programs

Tap a pack button to display its protocols.

Tap this button to return to the User Selection screen.

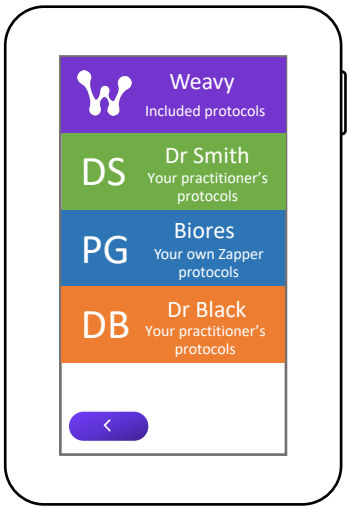


How To Get New Protocols

You can get new protocols in several ways:

- Consult one or more practitioners, who will create personalized protocols tailored to your needs.
- Explore and purchase Optimal Health programs to access additional protocols packs.
- Explore and purchase packs provided by our Optimal Health partners.

Once your new protocols are available for your Protocol Library, sync your Weavy® to download them.

Protocol Selection



Protocols with a purple background are FSM protocols.

Protocols with a light blue background are Zapper protocols.


Swipe up or down to scroll through the protocols.

AZ Tap this button to select a protocol by its first letter.

Tap a protocol to start it.

Tap this button to return to the Protocol Library.

Protocol List Mode

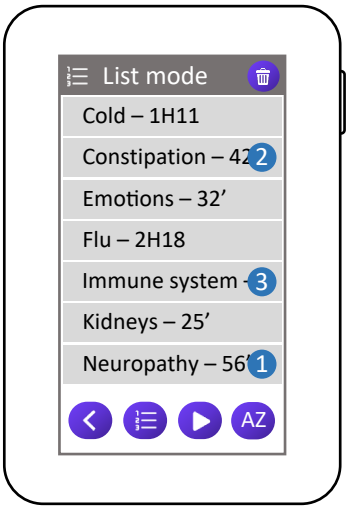

List mode allows you to create a list of up to 9 protocols to run automatically in your chosen order.

Tap this button to enter or exit List mode.


Tap a protocol to add it to the list.

Press and hold a protocol to remove it from the list.

Tap this button to run the protocols in the list.

Tap this button to clear the list.

Indicators




With an active Weavy Life subscription, your practitioners can use indicators for your follow-up.

When an indicator is set up for a protocol, this indicator screen will be displayed before or after running the protocol.

Simply slide to select your answer, then tap this button

Tap this button to return to the Protocol Selection screen.

Electrode Placement




Follow the instructions on the screen to place the electrodes.

Once the electrodes are in place, tap this button to start the protocol.

Tap this button to return to the Protocol Selection screen.

Run a Protocol

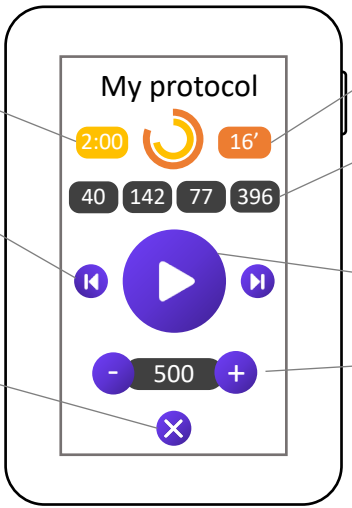

Remaining frequency time •

Previous / Next buttons •
Available only if enabled by your practitioner

Return to the protocol • selection screen


• Protocol time remaining

• Emitted frequencies
In Zapper mode, this area displays a progress bar

• Start / Stop button

• Increase / decrease the output intensity buttons
The displayed value is in µA or V, depending on the selected settings

Protocol Running – Sleep Screen



When a protocol is running, the screen automatically goes to sleep after 30 seconds.

This feature helps preserve battery life and extend the device's autonomy.

To wake the screen:

- Double-tap the screen
- Or, press the On/Off button

Troubleshooting

Device not responding	Press and hold the On/Off button for 5 seconds to force the device to shut down.
A message is displayed: "Power limit. Check the cable and electrode connections."	There may be several reasons: • The body is not sufficiently hydrated to allow the requested current to flow. • The electrodes are not conductive enough; check that they are properly positioned on the body over their entire surface. • The cable is disconnected. If the cable and electrodes are correctly positioned, try reducing the intensity.
New protocols do not appear	To receive new protocols, synchronize your Weavy®. Swipe down and tap the 'Synchronize' button.

Support

If you encounter any problems in using the product or need any help, please contact Perfect Waves Support Team via the following ways:


support@weavy.life


https://weavy.life/support

Statement:
All copyrights belong to Perfect Waves SL. Without the written approval of Perfect Waves SL, no organization or individual may copy or reproduce part or all of any written or illustrative content and disseminate it in any form.

Trademark statement:
All the trademarks are owned by Perfect Waves SL.

Note: Due to product version upgrades or others reasons this quick guide will be updated from time to time. Unless otherwise agreed, this document is provided as a guide for use only. All representations, information and recommendations in this document do not constitute warranties of any kind, express or implied.

Designed by

Perfect WAVES



Weavy®

Perfect Waves LLC
1501 S Greeley Hwy
Cheyenne, WY 82007
USA

Made in Spain